# Flowflex™ COVID-19 Antigen Home Test

Quick Reference Instructions

## 1 Wash

## 2 Prepare




## 3 Peel and Place



## 4 Open



## 5 Collect Sample

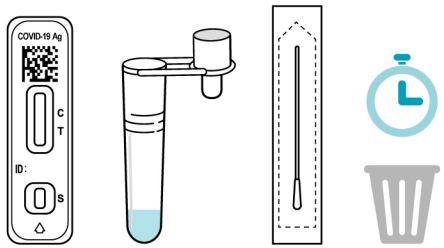


Insert | Swab | Remove

## 6 Prepare Sample

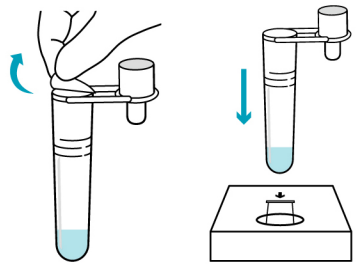


Swirl | Squeeze | Remove | Dispose
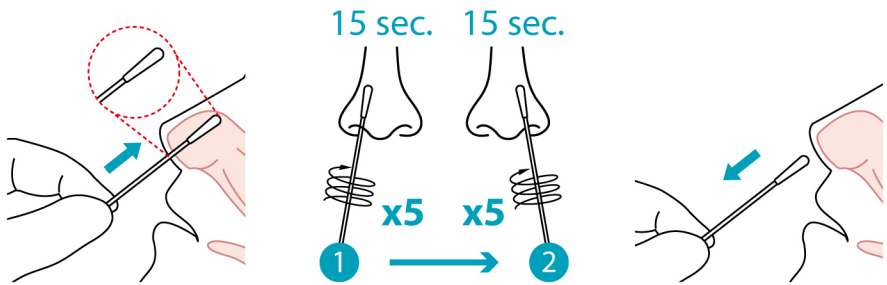
## 7 Process Sample




Cap | Dispense | Dispose
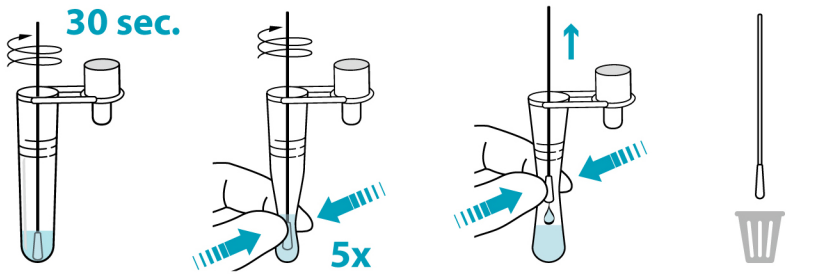
## 8 Wait

15 MIN

## 9 Read Result

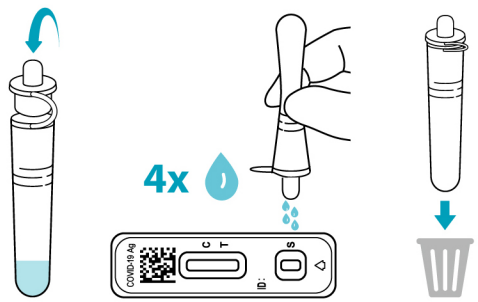


## 10 Dispose

**Repeat test using a new cassette**


ACON Laboratories, Inc.
San Diego, CA 92121, USA
Customer Support 1-800-838-9502
flowflexcovid.com

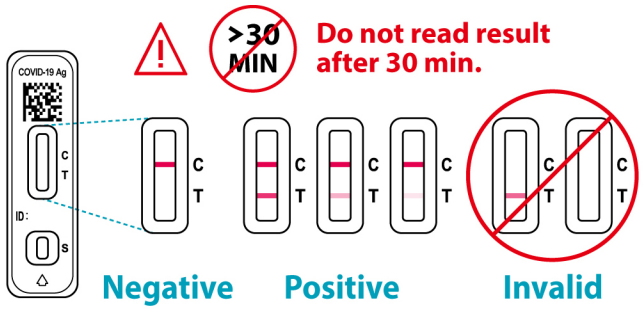

Number: 1151321501 Effective date: 2021-12-14